


Gastroenterology Product Catalog: Diagnostic Testing Systems

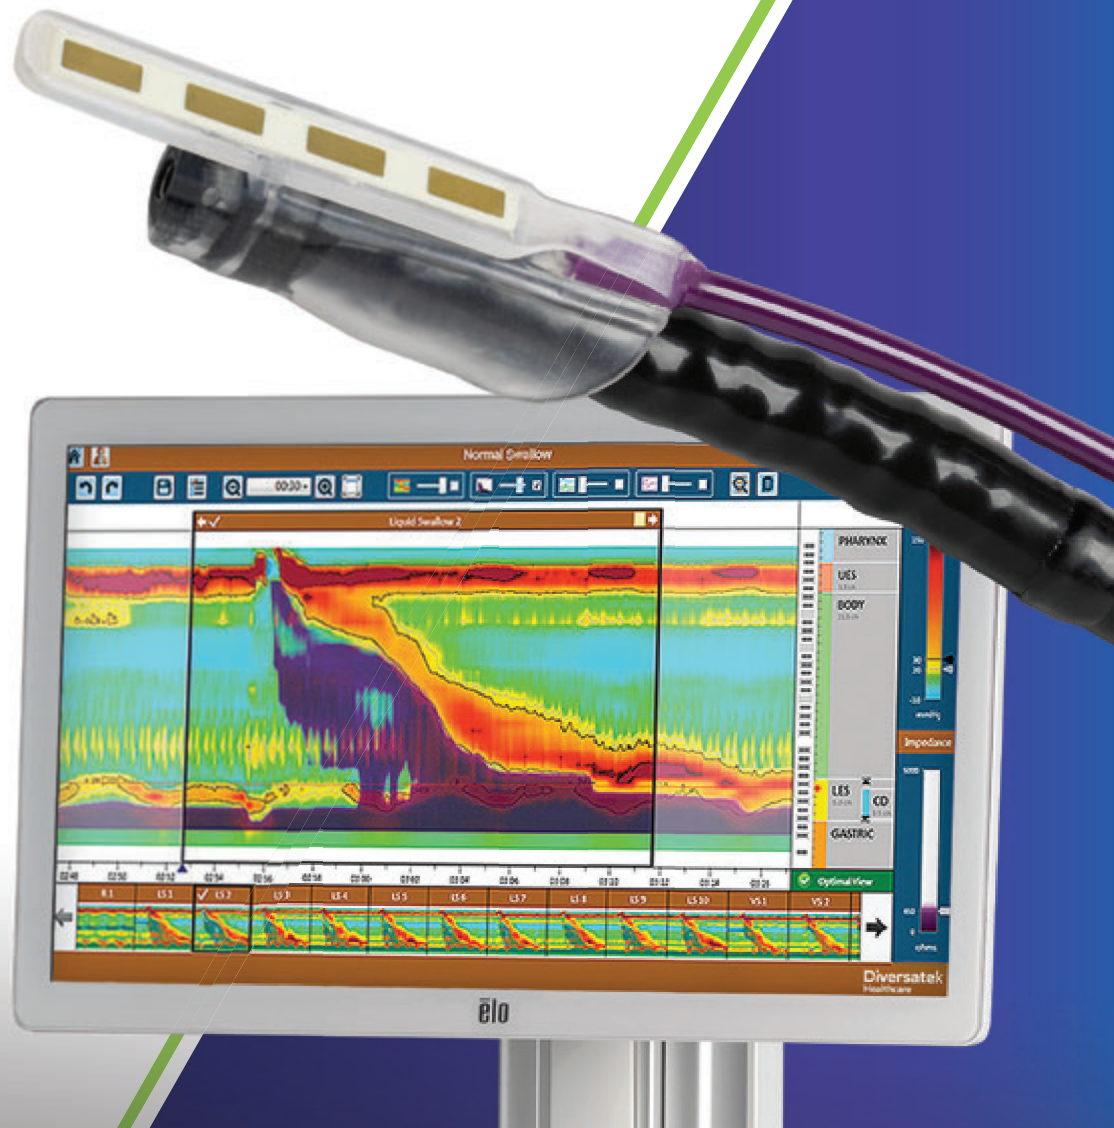

+1 800 558 6408 or +1 414 265 7620

Orders: orders@diversatekhc.com
General Inquiries: sales@diversatekhc.com

Global Corporate Office:
102 East Keefe Avenue
Milwaukee, WI 53212 USA

DiversatekHealthcare.com   

©2026 Diversatek, Inc. | All Rights Reserved. 080-0070 04/26

Access On-Demand
Education



diversateku.com

Scan to Order



Table of Contents: Testing Systems

Mucosal Integrity

MiVu™ Mucosal Integrity Testing System..... 1

Reflux Monitoring

ZepHr® Recorder & Accessories..... 2

ZepHr® Replacement Parts..... 2

Z/pH Probes..... 3

pH Probes..... 3

GI Motility

High Resolution Esophageal Manometry Base Design Options..... 4

High Resolution Esophageal Manometry Probes & Accessories..... 5

Pelvic Floor Evaluation

Anorectal Manometry Base Design Options..... 6

Anorectal Manometry Probes & Accessories..... 6-7

Computer Kits & Accessories

Replacement Computer Accessories..... 7

Product Training

Diversatek University Training..... 8

Mucosal Integrity

MiVu™ Mucosal Integrity Testing System for Use With MiVu™ Endo Cap

Choose a MiVu Base Design Option:

MiVu™ Base Option A: New User with No Existing Base System

For new users, who want to perform MiVu Mucosal Integrity Studies without an existing Base System

| Part No. | Description |
|--------------|---|
| PRIZMCART-II | PriZm® Base Cart System. Includes PriZm® Central Unit, 24" LCD medical grade monitor, computer, keyboard/mouse and printer, Zvu® and BioVIEW® Software. |

MiVu™ Base Option B: New User with No Existing Base System. Isolation Transformer Included.

For new users, who want to perform MiVu Mucosal Integrity Studies without an existing Base System – and includes an isolation transformer

| Part No. | Description |
|-------------|---|
| PRIZMSYS-II | PriZm® Base System. Includes PriZm® Central Unit, plus isolation transformer. |

MiVu™ Base Option C: Upgrade Option for Existing inSIGHT Ultima® User

For existing inSIGHT Ultima® Base Cart System (ULTCART) or inSIGHT Ultima® Base System (ULTSYS) users who want to perform MiVu™ Mucosal Integrity Studies

| Part No. | Description |
|--------------|---|
| PRIZMUPG-KIT | PriZm® Base System. Includes PriZm® Central Unit, Zvu® and BioVIEW® Software. |

MiVu™ Endo Cap & Accessories

| Part No. | Description | Qty/Case |
|---------------|---|----------|
| MI-ESO-CAP-3L | MiVu™ Esophageal Endo Cap. Compatible with an endoscope diameter of 9.9 mm (single-use, non-sterile). | 1 |
| MI-CAB-02 | MiVu™ Endo Cap Cable. Connects the MiVu™ Esophageal Endo Cap to the PriZm® Central Unit. | 1 |

MiVu™ Mucosal Integrity Testing System is covered by one or more of the following patents: US 11,291,382, US 9,814,408 and US 10,321,867.



Zvu® Software

GI Motility Software

Included in Base Options listed above

| Part No. | Description |
|-----------|--|
| ZVU-3 | Zvu® Software for MiVu™ Mucosal Integrity Studies, Reflux Monitoring, and Esophageal Manometry. Electronic delivery. |
| ZVU-3-ZIP | Zvu® Software for MiVu™ Mucosal Integrity Studies, Reflux Monitoring, and Esophageal Manometry. Zip drive. |

Reflux Monitoring (Impedance/pH)

ZepHr® Recorder & Accessories

ZepHr® Recorder


| Part No. | Product | Description | Qty/Case |
|-------------|----------------------|--|----------|
| Z07-2000B-B | ZepHr® Z/pH Recorder | For ambulatory impedance/pH reflux monitoring. Includes carrying case, two SD cards, and two AA batteries. Limited two year warranty | 1 |

ZepHr® Accessories

| Part No. | Product | Description | Qty/Case |
|------------|-------------------------------|--|----------|
| Z07-9000 | ZepHr® System Starter Kit | Includes an SD Card Reader, pH Calibration Tubes, and Buffer Solutions. Includes Zvu® Software | 1 |
| Z07-PACK | ZepHr® Pack | ZepHr® associated accessories | 1 |
| A04-2000-S | ZepHr® Sphincter Locator | LES locator for pH or Z/pH reflux testing. Infused probes are required for use. | 1 |
| D82-3103 | pH 1 Buffer Solution (500 mL) | For use with pH reflux testing system and probes | 1 |
| D82-3151 | pH 4 Buffer Solution (500 mL) | For use with Diversatek Healthcare Z/pH or pH reflux testing system and probes | 1 |
| D82-3152 | pH 7 Buffer Solution (500 mL) | For use with Diversatek Healthcare Z/pH or pH reflux testing system and probes | 1 |
| NG-25 | Nasal Tube Fastener | For reflux studies. Adult size | 25 |



ZepHr®
ZepHr® Z/pH Recorder
#Z07-2000B-B

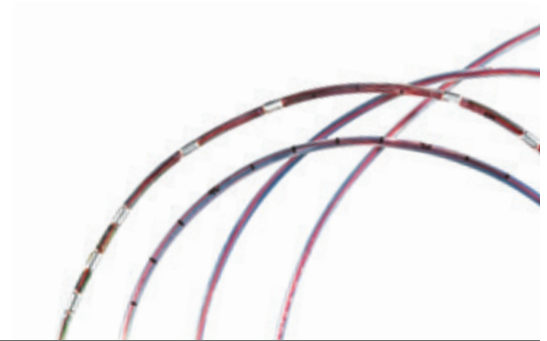

ZepHr® Replacement Products

ZepHr® Replacement Products

| Part No. | Description | Qty/Case |
|-------------|---|----------|
| Z07-4053 | ZepHr® Battery Cover | 1 |
| Z07-4055 | ZepHr® Probe Cover, Smoke | 1 |
| Z07R-8002 | ZepHr® Thermoform Pouch | 1 |
| Z07-1250 | SD Flash Memory Card | 1 |
| L89-5700-4 | USB Multicard Reader Kit for ZepHr® | 1 |
| L89-6020-40 | pH Calibration Tubes (Set of 3). Includes pH 4 and pH 7 buffer tubes, plus a water tube | 1 |
| L89-6021-40 | pH Calibration Buffer Tube, 40 cm. Includes both pH 4 and pH 7 labels | 1 |
| L89-8080 | pH Calibration Stand | 1 |
| L89-8081-40 | pH Calibration Water Tube, 40 cm | 1 |

Reflux Monitoring

Z/pH Probe

Z/pH Probe, Internal Reference, Non-infused

Single-use, Non-sterile

| Part No. | Description | Qty/Case |
|-----------|--|----------|
| ZAN-BS-01 | ≥ 18 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), 6.4 FR / 2.13 mm | 1 |
| ZAN-BD-31 | ≥ 18 cm Esophageal length, 6 impedance, 2 pH channels 0 & 15 cm (esophageal), 6.4 FR / 2.13 mm | 1 |
| ZAN-BG-44 | ≥ 18 cm Esophageal length, 6 impedance, 2 pH channels -15 & 0 cm (esophageal and gastric), 6.4 FR / 2.13 mm | 1 |
| ZPN-BG-07 | 15–18 cm Esophageal length, 6 impedance, 2 pH channels -12 & 0 cm (esophageal and gastric), 6.4 FR / 2.13 mm | 1 |
| ZPN-BS-46 | 15–18 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), 6.4 FR / 2.13 mm | 1 |
| ZPN-BS-50 | 15–18 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), 6.4 FR / 2.13 mm. Sensor spacing at 1.5 cm | 1 |
| ZPN-BG-57 | 15–18 cm Esophageal length, 6 impedance, 2 pH channels -7 & 0 cm (esophageal and gastric), 6.4 FR / 2.13 mm | 1 |
| ZIN-BS-51 | < 15 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), 6.4 FR / 2.13 mm | 1 |

Z/pH Probe, Internal Reference, Infused

Single-use, Non-sterile. Can be used with ZepHr® Sphincter Locator

| Part No. | Description | Qty/Case |
|-----------|--|----------|
| ZAI-BS-01 | ≥ 18 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), infusion port at 6 cm, 6.9 FR / 2.3 mm | 1 |
| ZAI-BD-31 | ≥ 18 cm Esophageal length, 6 impedance, 2 pH channels 0 & 15 cm (esophageal), infusion port at 6 cm, 6.9 FR / 2.3 mm | 1 |
| ZAI-BG-44 | ≥ 18 cm Esophageal length, 6 impedance, 2 pH channels -15 & 0 cm (esophageal and gastric), infusion port at 6 cm, 6.9 FR / 2.3 mm | 1 |
| ZPI-BS-46 | 15–18 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), infusion port at 6 cm, 6.9 FR / 2.3 mm | 1 |
| ZPI-BG-52 | 15–18 cm Esophageal length, 6 impedance, 2 pH channels -12 & 0 cm (esophageal and gastric), infusion port at 6 cm, 6.9 FR / 2.3 mm | 1 |

LPR Probe, Internal Reference, Infused

Single-use, Non-sterile. Can be used with ZepHr® Sphincter Locator

| Part No. | Description | Qty/Case |
|-----------|--|----------|
| ZAI-BL-54 | 26–28 cm Esophageal length, 2 pH channels -25 & 0 cm (UES), infusion port at 6 cm (above UES), 6.9 FR / 2.3 mm | 1 |
| ZAI-BL-55 | 23–25 cm Esophageal length, 2 pH channels -22 & 0 cm (UES), infusion port at 6 cm (above UES), 6.9 FR / 2.3 mm | 1 |
| ZAI-BL-56 | 20–22 cm Esophageal length, 2 pH channels -19 & 0 cm (UES), infusion port at 6 cm (above UES), 6.9 FR / 2.3 mm | 1 |

Z/pH Probe, External Reference, Non-infused

Single-use, Non-sterile

| Part No. | Description | Qty/Case |
|------------|--|----------|
| ZAN-BS-01E | ≥ 18 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), 6.4 FR / 2.13 mm | 1 |
| ZPN-BS-46E | 15–18 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), 6.4 FR / 2.13 mm | 1 |
| ZIN-BS-45E | < 15 cm Esophageal length, 6 impedance, 1 pH channel (esophageal), 6.4 FR / 2.13 mm | 1 |

pH Probe

pH Probe, Internal Reference, Non-infused

Single-use, Non-sterile

| Part No. | Description | Qty/Case |
|----------|---|----------|
| PHNS-P | 1 pH channel, 5 FR / 1.67 mm | 1 |
| PHNS | 1 pH channel, 6.4 FR / 2.13 mm | 1 |
| PHN5 | 2 pH channels 0 & 5 cm, 6.4 FR / 2.13 mm | 1 |
| PHN10-P | 2 pH channels 0 & 10 cm, 5 FR / 1.67 mm | 1 |
| PHN10 | 2 pH channels 0 & 10 cm, 6.4 FR / 2.13 mm | 1 |
| PHN15 | 2 pH channels 0 & 15 cm, 6.4 FR / 2.13 mm | 1 |
| PHN21 | 2 pH channels 0 & 21 cm, 6.4 FR / 2.13 mm | 1 |

pH Probe, Internal Reference, Infused


Single-use, Non-sterile. Can be used with ZepHr® Sphincter Locator

| Part No. | Description | Qty/Case |
|----------|---|----------|
| PHIS | 1 pH channel, infusion port at 5 cm, 6.9 FR / 2.3 mm | 1 |
| PHI10 | 2 pH channels 0 & 10 cm, infusion port at 5 cm, 6.9 FR / 2.3 mm | 1 |
| PHI15 | 2 pH channels 0 & 15 cm, infusion port at 5 cm, 6.9 FR / 2.3 mm | 1 |

Zvu® Software

GI Motility Software

| Part No. | Description |
|-----------|--|
| ZVU-3 | Zvu® Software for MiVu™ Mucosal Integrity Studies, Reflux Monitoring, and Esophageal Manometry. Electronic delivery. |
| ZVU-3-ZIP | Zvu® Software for MiVu™ Mucosal Integrity Studies, Reflux Monitoring, and Esophageal Manometry. Zip drive. |

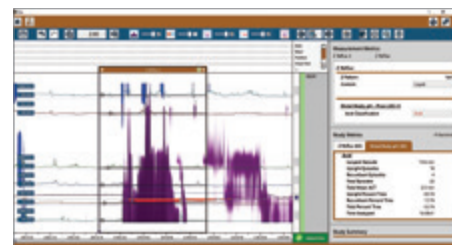

Zvu® Software
#ZVU-3



High Resolution Esophageal Manometry

Choose a Manometry Base Design Option:

Manometry Base Option A: New User with No Existing Base System

For new users who want to perform High Resolution Manometry or MiVu™ Mucosal Integrity Studies, without an existing Base System

| Part No. | Description |
|--------------|---|
| PRIZMCART-II | PriZm® Base Cart System. Includes PriZm® Central Unit, 24" LCD medical grade monitor, computer, keyboard/mouse and printer. |
| MANO-KIT | Manometry Starter Kit. For customers with an existing inSIGHT Ultima® or PriZm® System. Includes air and water calibration kits, plus connecting tubing to the PriZm® Base Cart System. Includes Zvu® and BioView® Software |



PriZm® Gen-II
Central Unit

PriZm®

Manometry Base Option B: New User with No Existing Base System. Isolation Transformer Included.

For new users who want to perform High Resolution Manometry or MiVu™ Mucosal Integrity Studies, without an existing Base System – and include an isolation transformer.

| Part No. | Description |
|-------------|--|
| PRIZMSYS-II | PriZm® Base System. Includes PriZm® Central Unit plus isolation transformer |
| MANO-KIT | Manometry Starter Kit. For customers with an existing inSIGHT Ultima® or PriZm® System. Includes air and water calibration kits, plus connecting tubing to the PriZm® Base Cart System. Includes Zvu® and BioView® Software. |

Manometry Base Option C: Upgrade Option for Existing inSIGHT Ultima® User


For existing inSIGHT Ultima® Base Cart System (ULTCART) or inSIGHT Ultima® Base System (ULTSYS) users who want to perform High Resolution Manometry and have access to MiVu™ functionality.

| Part No. | Description |
|--------------|---|
| PRIZMUPG-KIT | PriZm® Base System. Includes PriZm® Central Unit, Zvu® and BioVIEW® Software. |

Manometry Base Option D: New User with No Existing Base System

For new users who want to perform High Resolution Manometry. This option is not compatible for MiVu™ Mucosal Integrity Studies.

| Part No. | Description |
|----------|--|
| ULTCART | inSIGHT Ultima® Base Cart System. Includes inSIGHT Ultima® Central Unit, 24" LCD medical grade monitor, computer, keyboard/mouse and printer. Motility Cart with isolation transformer |
| MANO-KIT | Manometry Starter Kit. For customers with an existing inSIGHT Ultima® or PriZm® System. Includes air and water calibration kits, plus connecting tubing to the inSIGHT Ultima® or PriZm® Base Cart System. Includes Zvu® and BioView® Software |

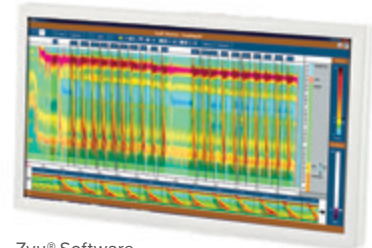

Zvu® Software
#ZVU-3

Zvu®

Manometry Base Option E: New User with No Existing Base System

For new users who want to perform High Resolution Manometry without an existing Base System. This option is not compatible for MiVu™ Mucosal Integrity Studies.

| Part No. | Description |
|----------|--|
| ULTSYS | inSIGHT Ultima® Base System. Includes inSIGHT Ultima® Central Unit plus isolation transformer. • Motility Cart and computer/monitor not included |
| MANO-KIT | Manometry Starter Kit. For customers with an existing inSIGHT Ultima® or PriZm® System. Includes air and water calibration kits, plus connecting tubing to the inSIGHT Ultima® or PriZm® Base Cart System. Includes Zvu® and BioView® Software |

GI Motility Software

Included in Base Options listed above

| Part No. | Description |
|-----------|--|
| ZVU-3 | Zvu® Software for MiVu™ Mucosal Integrity Studies, Reflux Monitoring, and Esophageal Manometry. Electronic delivery. |
| ZVU-3-ZIP | Zvu® Software for MiVu™ Mucosal Integrity Studies, Reflux Monitoring, and Esophageal Manometry. Zip drive. |

High Resolution Esophageal Manometry

Probe Kits for PriZm® Esophageal Manometry Systems

Motility cart, computer, monitor, and software not included

| Part No. | Description | Qty/Case |
|-------------------|--|----------|
| HRIM-201-12-KIT * | Zvu® High Resolution Esophageal Manometry Probe Kit (34 circumferential pressure / 18 impedance channels. 12 FR. Part #HRIM-201), plus appropriate cable | 1 |

Esophageal Manometry Probes


| Part No. | Description | Qty/Case |
|------------|--|----------|
| HRIM-201 * | Zvu® HRiM Esophageal Manometry Probe. 34 circumferential pressure / 18 impedance channels. 12 FR | 1 |

Esophageal Manometry Accessories

| Part No. | Description | Qty/Case |
|-------------|--|----------|
| EFTV-12V | Viscous Solution, 80 mL containers. Used with esophageal probes utilizing impedance technology | 12 |
| H12R-5100 | Air Calibration Tube Kit, 18" for inSIGHT Ultima® and PriZm® | 1 |
| H12R-5200 | Water Calibration Tube Kit for inSIGHT Ultima® and PriZm® | 1 |
| H12R-5400 | Auto Calibration Air Lines Kit for Zvu® Software, PriZm®, and inSIGHT Ultima® | 1 |
| H12R-7110 | inSIGHT Ultima® and PriZm® Cable for Unisensor Probe | 1 |
| H12R-7610 * | Cable for Zvu® HRiM and HRaM Probes | 1 |
| ISO-MED-3 | Isolation Transformer | 1 |
| S90-5120-H | Calibration Tube Universal Washer and O-Ring Replacement Kit | 1 |



Zvu® HRiM Esophageal Manometry Probe
#HRIM-201

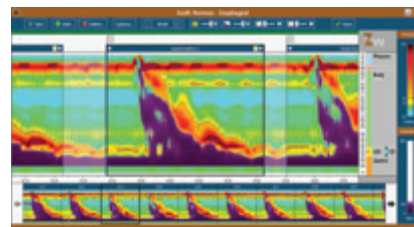

Zvu® Software
#ZVU-3



*Zvu® software version 3.0 or higher is required.

Pelvic Floor Evaluation

Anorectal Manometry

Choose a Manometry Base Design Option:

Manometry Base Option A: New User with No Existing Base System

For new users who want to perform High Resolution Manometry or MiVu™ Mucosal Integrity Studies, without an existing Base System

| Part No. | Description |
|--------------|---|
| PRIZMCART-II | PriZm® Base Cart System. Includes PriZm® Central Unit, 24" LCD medical grade monitor, computer, keyboard/mouse and printer. |
| MANO-KIT | Manometry Starter Kit. For customers with an existing inSIGHT Ultima® or PriZm® System. Includes air and water calibration kits, plus connecting tubing to the PriZm® Base Cart System. Includes Zvu® and BioView® Software |



PriZm® Gen-II
Central Unit

PriZm®

Manometry Base Option B: New User with No Existing Base System. Isolation Transformer Included.

For new users who want to perform High Resolution Manometry or MiVu™ Mucosal Integrity Studies, without an existing Base System – and include an isolation transformer.

| Part No. | Description |
|-------------|--|
| PRIZMSYS-II | PriZm® Base System. Includes PriZm® Central Unit plus isolation transformer |
| MANO-KIT | Manometry Starter Kit. For customers with an existing inSIGHT Ultima® or PriZm® System. Includes air and water calibration kits, plus connecting tubing to the inSIGHT Ultima® or PriZm® Base Cart System. Includes Zvu® and BioView® Software |

Manometry Base Option C: Upgrade Option for Existing inSIGHT® Ultima User

For existing inSIGHT Ultima® Base Cart System (ULTCART) or inSIGHT Ultima® Base System (ULTSYS) users who want to perform High Resolution Manometry and have access to MiVu™ functionality.

| Part No. | Description |
|--------------|---|
| PRIZMUPG-KIT | PriZm® Base System. Includes PriZm® Central Unit, Zvu® and BioVIEW® Software. |

Manometry Base Option D: New User with No Existing Base System

For new users who want to perform High Resolution Manometry. This option is not compatible for MiVu™ Mucosal Integrity Studies.

| Part No. | Description |
|----------|--|
| ULTCART | inSIGHT Ultima® Base Cart System. Includes inSIGHT Ultima® Central Unit, 24" LCD medical grade monitor, computer, keyboard/mouse and printer. Motility Cart with isolation transformer |
| MANO-KIT | Manometry Starter Kit. For customers with an existing inSIGHT Ultima® or PriZm® System. Includes air and water calibration kits, plus connecting tubing to the inSIGHT Ultima® or PriZm® Base Cart System. Includes Zvu® and BioView® Software |



Zvu® HRaM Anorectal Manometry Probe
#HRAM-200

Manometry Base Option E: New User with No Existing Base System

For new users who want to perform High Resolution Manometry without an existing Base System. This option is not compatible for MiVu Mucosal Integrity Studies.

| Part No. | Description |
|----------|--|
| ULTSYS | inSIGHT Ultima® Base System. Includes inSIGHT Ultima® Central Unit plus isolation transformer. Motility Cart and computer/monitor not included. |
| MANO-KIT | Manometry Starter Kit. For customers with an existing inSIGHT Ultima® or PriZm® System. Includes air and water calibration kits, plus connecting tubing to the inSIGHT Ultima® or PriZm® Base Cart System. Includes Zvu® and BioView® Software |

Probe Kits for Anorectal Manometry Systems

Choose Probe Kit(s):

| Part No. | Description |
|-----------------|---|
| HRAM-200-17-KIT | Zvu® High Resolution Anorectal Manometry Probe Kit (26 unidirectional pressure / 1 directional balloon channel. 16.7 FR. Part #HRAM-200). • Plus appropriate cables, ligator, anorectal balloon procedure kit • BioVIEW® Software included • Motility Cart, computer, and monitor not included |
| EMG-KIT | Anal Sphincter Electromyography Kit includes EMG Adapter, cables and perianal sensor • Motility Cart, computer, monitor, and software not included |

Anorectal Manometry Probes


| Part No. | Description |
|----------|--|
| HRAM-200 | Zvu® HRaM Anorectal Manometry Probe. 26 Unidirectional pressure / 1 balloon pressure channels. 16.7 FR |

Pelvic Floor Evaluation

Anorectal Manometry

GI Motility Software


| Part No. | Description | Qty/Case |
|--------------|--|----------|
| S98-1925-P1 | BioVIEW® Software for Anorectal Studies | 1 |
| S96-1118 | Data Extraction Utility Software Kit (compatible only with BioVIEW® software) | 1 |
| HRAM-100 | London Protocol Update, electronic delivery (compatible only with BioVIEW® software) | 1 |
| HRAM-100-ZIP | London Protocol Update, Zip drive (compatible only with BioVIEW® software) | 1 |

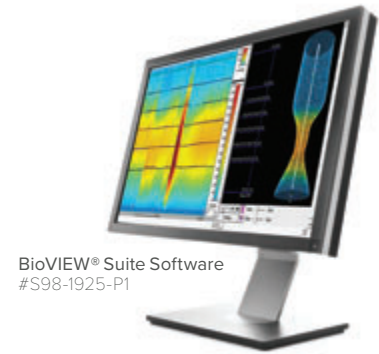

BioVIEW® Suite Software
#S98-1925-P1

Anorectal Manometry Accessories

| Part No. | Description | Qty/Case |
|--------------|--|----------|
| A86-1070 | Anorectal Balloon, adult, contains Latex. For anorectal compliance testing | 5 |
| A86-4100 | Polyurethane Bands (disk of 20 bands), for Unisensor HRaM Probes | 1 |
| A86-4110-10 | HRaM Kit. Includes 10 Anorectal Balloons, 20 Polyurethane Bands, and a Suture Removal Kit, for Unisensor HRaM Probes | 1 |
| A86-4120 | HRaM Syringe/Stopcock Kit | 1 |
| A86-4200 | Ligator for Unisensor HRaM Probes | 1 |
| A86-4300-10 | Anorectal Balloon, 400CC TPE, for Unisensor HRaM Probes | 10 |
| A86-4500 | Disposable Suture Removal Kit for Unisensor HRaM Probes | 1 |
| A86-5070 | Anorectal Balloon, small. Contains Latex | 5 |
| A97-1000 | StimSense Pressure Sensor. Measures rectal balloon pressure during anorectal compliance testing | 1 |
| H12R-4300 | EMG Adapter Assembly. Connects to the inSIGHT Ultima® and PriZm® | 1 |
| H12R-5400 | Auto Calibration Air Lines Kit for Zvu® Software, PriZm®, and inSIGHT Ultima® | 1 |
| H12R-7110 | Ultima® and PriZm® Cable for Unisensor High Resolution Manometry Probe | 1 |
| H12R-7210 | Ultima® and PriZm® Cable for HRCA Manometry Probe (Lemo Connector) | 1 |
| H12R-7610 | Cable for Zvu® HRiM and HRaM Probes | 1 |
| HRAM-BAL-10 | Anorectal Balloon for Zvu® HRaM Probes, 400CC TPE, and Balloon Retention Bands | 10 |
| HRAM-LIGATOR | Zvu® Ligator. For balloon attachment to a Zvu® HRaM Probe | 1 |
| HRAM-PROC-10 | Zvu® Anorectal Balloon Attachment & Removal Kit (single-use). Includes Zvu® Anorectal Balloons, Balloon Retention Bands, Band EZ-Remove Guides, and disposable scalpel | 10 |
| ISO-MED-3 | Isolation Transformer | 1 |
| SRS-4510 | Perianal Rectal Sensor (single-use) | 1 |
| SR1B | Mui Scientific Anorectal Expulsion Balloon Catheter (single-use) | 10 |

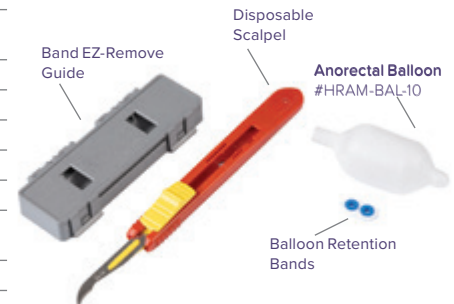

Zvu® Anorectal Balloon Attachment & Removal Kit
(All Items Shown Above)
#HRAM-PROC-10



Zvu® Ligator
#HRAM-LIGATOR

Computer Kits & Accessories

Replacement Computer Kits & Accessories

For inSIGHT Ultima® and PriZm® Systems

| Part No. | Description | Qty/Case |
|-------------|---|----------|
| COMP-KIT | Desktop PC with Windows 10. Includes a wireless keyboard and mouse • Installed with Zvu® and BioVIEW® Software | 1 |
| L89-5355 | Printer USB Cable | 1 |
| L89-5500 | Desktop Color Printer | 1 |
| SYS-MONITOR | Monitor, Touchscreen LCD, 24" for inSIGHT Ultima® and PriZm® | 1 |

Service Agreements

Service Agreements for Diagnostic Equipment

| Part No. | Description | Qty |
|-----------------|---|-----|
| SVC-AGR-CART-W | 3-year Service Agreement with Computer and Monitor | 1 |
| SVC-AGR-CART-WO | 3-year Service Agreement without Computer and Monitor | 1 |
| SVG-AGR-PZM | 3-year Service Agreement—PriZm Upgrade | 1 |
| SVG-AGR-Z07 | 3-year Service Agreement—Recorder | 1 |

Product Training

Product Training at Diversatek University Denver & Onsite

Product Training at Diversatek University Denver

| Part No. | Description | Qty |
|----------|--|-----|
| DEN-FGID | <ul style="list-style-type: none">• One Registration—3 Day Functional GI Diagnostic Training• Training on High Resolution Esophageal Manometry, Reflux Studies, and Anorectal Manometry• Location: Denver• Expires 1 year from Invoice Date (Does not include transportation/hotel costs) | 1 |

Onsite Clinical Training

- Includes one set of master manuals
- Expires 1 year from Invoice Date

| Part No. | Description | Qty |
|----------------|--|-----|
| ON-SITE-ANO | Clinical Training Onsite (Two Day Session)—High Resolution Anorectal Manometry | 1 |
| ON-SITE-ESO | Clinical Training Onsite (Two Day Session)— High Resolution Esophageal Manometry | 1 |
| ON-SITE-REFLUX | Clinical Training Onsite (One Day Session)—Reflux Testing | 1 |

Virtual Training

| Part No. | Description | Qty |
|--------------|-----------------------------------|-----|
| VIRT-FULLDAY | Full Day Virtual Training Session | 1 |
| VIRT-HALFDAY | Half Day Virtual Training Session | 1 |



Your Expertise Drives Exceptional GI Care

Diversatek University (DU) offers comprehensive education and training, online, on-site, and in-person, to ensure your team receives a personalized learning experience that supports your goals and enhances clinical confidence.

DiversatekU.com

To place an order, call **+1 800 558 6408**
or email orders@diversatekhc.com

DiversatekHealthcare.com

